



PA30IS Series Powered Air-Purifying Respirator PA3IS Blower Assembly User Manual

With High Efficiency (HE) Filters (2) - Approval No. TC-21C-0796/TC-21C-0825
With OV-AG-HE Cartridges (3) for organic vapors, chlorine, hydrogen chloride, sulfur dioxide, chlorine dioxide or hydrogen fluoride and particulates - Approval No. TC-23C-2307/TC-23C-2384

With PA3NBC cartridges (3) for chlorine, hydrogen chloride, sulfur dioxide, chlorine dioxide, hydrogen fluoride, ammonia, methylamine, and particulates - Approval No. TC-23C-2306

PA30IS PAPR

Cautions and Limitations

- A. Not for use in atmospheres containing less than 19.5% oxygen.
- B. Not for use in atmospheres immediately dangerous to life or health.
- C. Do not exceed maximum use concentrations established by regulatory standards.
- F. Do not use respirator if airflow is less than four cfm (115 lpm) for tight fitting face pieces or six cfm (170 lpm) for hoods and/or helmets.
- H. Follow established cartridge and canister change schedules or observe ESLI to ensure that cartridges and canisters are replaced before breakthrough.
- I. Contains electrical parts that may cause an ignition in flammable or explosive atmospheres.
- J. Failure to properly use and maintain this product could result in injury or death.
- K. The Occupational Safety and Health Administration regulations require gas-proof goggles to be worn with this respirator when used against formaldehyde.
- L. Follow the manufacturer's user instructions for changing cartridges and/or filters.
- M. All approved respirators shall be selected, fitted, used and maintained in accordance with MSHA, OSHA and other applicable regulations.
- N. Never substitute, modify, add or omit parts. Use only exact Bullard replacement parts in the configuration as specified by the manufacturer.
- O. Refer to User's Instructions and/or maintenance manuals for information on use and maintenance of these respirators.
- P. NIOSH does not evaluate respirators for use as surgical masks.

The PA3IS PAPR Blower is Factory Mutual (FM) approved for
CLASS I DIV 1 Groups C, D
CLASS II DIV 1 Groups E, F, G
CLASS III DIV 1
Ta = -12°C to 49°C T4

Table of Contents

Warnings, Cautions and Limitations	1	Mounting and Replacing Cartridges	5
Principle of Operation	2	Donning the Blower	5
Battery Pack	2	Low Battery Alarm	6
Pre-Operational Inspection	3	Troubleshooting	6
Mounting the Breathing Tube	3	Cleaning and Storage	6
Checking Air Flow	3	Niosh Approval Label	7
Air-Purifying Elements	4	Ordering Information	8

⚠ WARNING

Use strictly in accordance with instructions, labels and limitations pertaining to the PA30IS respirator.

1. The PA30IS respirator does not supply oxygen. Use only in adequately ventilated areas containing at least 19.5% oxygen.
 2. Do not use when concentrations of contaminants are immediately dangerous to life or health (IDLH). This term is defined in 29CFR 1910.134 (b).
 3. Do not use these respirators for respiratory protection during abrasive blasting or clean up.
 4. Do not use in circumstances where the airborne concentration level of contaminant exceeds maximum use concentration for this type of respirator as established by regulatory standards.
 5. Leave area immediately if:
 - Breathing becomes difficult
 - Dizziness or other distress occurs
 - You taste or smell the contaminant
 - Unit becomes damaged
 - Voltage alarm activates
 6. This apparatus must not be worn with the blower unit switched off. If the blower is switched off, a rapid build-up of carbon dioxide and depletion of oxygen may occur, which could result in death or serious injury.
 7. Never alter or modify this respirator. Use only Bullard NIOSH-approved PA30IS components and replacement parts for this respirator.
- Failure to follow these warnings could result in death or serious injury.

PA3IS - Principle of Operation

The PA30IS Powered Air-Purifying Respirator (PAPR) System is supplied in six parts:

- The blower assembly (Part No. PA3IS) which includes:
 - PA3ISBU Blower Unit
 - PA1SB Belt or PA1DB Decon Belt
 - PA1AFI Air Flow Indicator
- The battery pack, Part No. PA3ISBP, will last approximately seven hours.
- The breathing tube, which is available in two different types:
 - PA1BT Hood Breathing Tube Assembly with Clamp (Standard Length)
 - PA1BTXS Hood Breathing Tube Assembly with Clamp (Short Length)
 - PA20LFBT Loose Fitting Facepiece Breathing Tube Assembly (Standard Length)
 - PA20LFBTXS Loose Fitting Facepiece Breathing Tube Assembly (Short Length)
 - PA20LFBTXL Loose Fitting Facepiece Breathing Tube Assembly (Extra Long Length)
- The cartridges are available in different types for most toxic contaminants. (See pages 4 and 7 for a listing of the cartridges.) The types include High Efficiency particulate only, chemical cartridges for gases and vapors, and combination cartridges for gases, vapors and particulates.
- The hood with headband suspension and/or hard hat, or loose fitting facepiece. The following hood models may be used with the PA3ISBU blower unit:
 - RT1/RT2 Hood with long inner and outer bib (inflatable neck cuff)
 - RT3/RT4 Hood with long inner and outer bib (sport neck cuff)
 - 20TJ Hood
 - 20TIC Hood with Inner Bib
 - 20TICH Hood for use with Bullard Hard Hat
 - 20TICS Hood with Taped and Sealed Seams
 - 20SIC Hood with Taped and Sealed Seams
 - 20SICV Hood with Taped and Sealed Seams and CBRN-resistant PVC lens
 - 20SICH Hood with Taped and Sealed Seams for use with Bullard Hard Hat
 - 20SICVH Hood with Taped and Sealed Seams and CBRN-resistant PVC lens for use with Bullard Hard Hat
 - 20TPC Hood with Solvent Resistant Lens and Inner Bib
 - 20TP Hood with Solvent Resistant Lens
 - 20LFM Loose Fitting Facepiece, Medium Size
 - 20LFL Loose Fitting Facepiece, Large Size
 - 20LF2L Loose Fitting Facepiece, Narrow Profile, Large Size
 - 20LF2M Loose Fitting Facepiece, Narrow Profile, Medium Size
 - 20LF2S Loose Fitting Facepiece, Narrow Profile, Small Size
- The Battery Charger:
 - PA3ISC Intrinsically Safe Quick Charger
 - PA3ISGC Intrinsically Safe Gang Charger

The blower unit draws in ambient air through the cartridges. The purified air is blown into the wearer's hood through the breathing tube. A flow indicator is provided to check that there is an adequate volume of air available to the wearer prior to use.

The units are designed for use at temperatures from 10°F to 120°F (-12°C to 49°C).

The system is designed to operate at a minimum air flow of approximately seven cubic feet of air per minute (210 liters per minute) in the hood under normal use.

The battery pack(s) mount in compartment(s) on the back of the blower. One fully charged battery pack will power the blower for approximately seven hours.

The PA3ISBU is fitted with an alarm which will sound when voltage is low.

CC20 and RT Series Airline Respirator

NIOSH Approval No. TC-19C-154, Type C and TC-19C-412, Type C

Most of the same headpieces approved for use with the CC20 and RT Series of supplied air respirators (SARS) are also approved for use with the PA30 Series of powered air-purifying respirators. CC20 and RT Series respirators provide a high level of respiratory protection and user comfort over long work periods, in a wide variety of hazardous environments.

The CC20 and RT SAR air flow control devices and other components are described in the CC20 and RT Series User Instructions.

Battery Pack

A fully charged battery pack will power a blower unit to provide adequate air volume for the respirator for approximately seven hours for the PA3ISBU.

To charge the battery pack, do the following:

- Open the battery latch and remove the battery from the back of the blower.

⚠ WARNING

Make sure that the Blower Unit has been shut off completely before removing the battery. DO NOT remove the battery while the unit is running. DO NOT install a battery into a blower that has been left in the "on" position. Failure to follow these instructions may cause damage to the battery and may put the wearer at risk.

- Place each battery in the charging ports of the battery charger. Ensure that the battery contacts line up with the contacts in the charger port (**see Figure 1**).
- Connect the battery charger to a 115-volt AC electrical outlet.

Charge the battery pack for approximately eight hours.

While the PA3ISBP battery is charging, the light on the cord will remain red. When the unit is charged, it will turn green.

Table-top gang chargers (Part No. PA3ISGC, with 6 ports) and analyzers/conditioners are also available.

To maximize battery life, these guidelines should be followed:

- Charge the battery pack before it is completely discharged. The low voltage alarm indicates that the battery needs to be charged.; operating the PAPR for more than 20 minutes after the alarm has been activated may damage the battery. Deeply discharged batteries may cause the charger to falsely indicate a complete charge.
- Always charge the batteries at room temperature or less. At higher temperatures, the battery pack may not accept a full charge. If the battery pack feels hot, let it cool for 30 minutes before charging.
- Do not charge battery packs in an enclosed cabinet without ventilation.
- Battery capacity may be checked with battery analyzer/conditioner.

Table-top gang chargers (Part No. PA3ISGC, with 6 ports) are also available.

⚠ WARNING

PA3BP battery packs MUST be used with PA3 blower units and PA3ISBP intrinsically safe battery packs MUST be used with PA3IS blower units. Interchanging these batteries with blowers may cause damage to the blower and battery AND the blowers will not operate as intended and may put the wearer at risk. Failure to follow these instructions may result in death or serious injury.



Figure 1

PA30IS Series Powered Air-Purifying Respirator PA3IS Blower Assembly User Manual

Initial Charging Procedure with Quick Charger

To ensure a full charge on a new battery pack, follow these important guidelines. These guidelines also apply to battery packs that have been in storage for extended periods of time.

For new battery packs or packs that have been in storage for extended periods of time, follow the directions above under "Battery Pack", and when the light turns green (PA3ISBP), do the following:

- Remove the battery pack. Wait 15 seconds. Replace the battery pack in the nest. The charger light will now turn red (PA3ISBP).
- When the light turns green (PA3ISBP), remove the battery pack. Wait 15 seconds. Replace the battery pack in the nest again. The charger light will now remain on or turn red.

The charger light will turn green (PA3ISBP), indicating that the battery is fully charged.

This procedure should also be followed after periods of prolonged storage. Without periodic charging, the nickel metal hydride batteries will lose up to 1%–2% of their charge per day. Allowing a battery to self-discharge during periods of prolonged storage will not damage the battery.

⚠ WARNING

DO NOT charge batteries in hazardous area.

Pre-Operational Inspection

Prior to each work shift, perform the following Pre-Operational Inspection to ensure proper operation and to insure that the unit is complete.

1. Belt Mounted Blower Unit, Part No. PA3ISBU

- Check that the unit is clean and undamaged.
- Inspect for deterioration, physical damage, and improper assembly.
- Ensure that the correct filters/cartridges for the appropriate contaminant are properly mounted on the blower unit. Screw the cartridges into the ports until hand-tight.

Consult the NIOSH approval label and your own in-plant safety professional if you have any questions as to the suitability and efficiency of the Air-Purifying Element.

2. Battery Pack

- Check that the battery is not damaged.
- Place the battery pack in the battery compartment on the blower by first engaging the tab on the pack under the lip on the edge of the compartment. Then close the latch.

3. Hood with Suspension or Hard Hat, or Loose Fitting Facepiece

- The hood is constructed of either Tychem QC or Tychem SL. Depending on the model selected, it may be used with either a headband suspension or a hard hat. The loose fitting facepiece is constructed of Tychem QC and features an internal suspension.
- All hoods and loose fitting facepieces are approved for use with the PA3ISBU Blower Units.
- Inspect the hood or loose fitting facepiece for any physical damage.

Mounting the Breathing Tube on the PA3ISBU Blower

Ensure that a rubber gasket is in place in the breathing tube coupler on the blower unit.

Screw one end of the breathing tube into the blower unit (hand tight is sufficient) (see Figure 2).

Ensure that neither the breathing tube nor the filter is blocked.

Ensure that the ON/OFF Switch is in the OFF position.

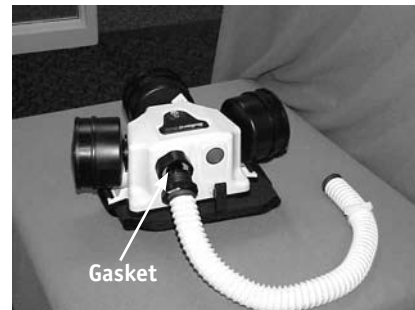


Figure 2

Switch on the blower. If the Low Voltage Alarm sounds at this time, the battery needs to be recharged. See instructions on page 4 regarding properly charging the battery.

Checking Airflow with the Airflow Indicator (PA1AFI)

With the blower switched ON and the filters/cartridges mounted, take the free end of the breathing tube in one hand, hold it upright and place the Airflow Indicator into the end of the tube (see Figure 3).

Apply a light downward pressure to the Airflow Indicator to get a reasonable seal at the breathing tube end. Ensure that the air outlet holes in the Airflow Indicator tube are not blocked. Two hands may be used if preferred, one to hold the breathing tube and one to hold the Airflow Indicator.



Figure 3

The position of the ball in the Airflow Indicator should be observed. If any part of the ball is below the PASS LINE on the Airflow Indicator, check for:

- Blower malfunction.
- Clogged or damaged Air-Purifying filter elements on the HE filters or the combination cartridges with HE filters. See "Mounting and Replacing Cartridges on the Blower Unit" on page 5.
- Low voltage or battery malfunction.

If the ball is completely above the PASS LINE on the Airflow Indicator, then the system is ready for use.

When the blower passes the flow test, it is ready to use.

⚠ WARNING

If the blower malfunctions during use in a hazardous area:

DO NOT remove the respirator hood, blower or waist-belt while in the hazardous area.

DO remain calm and **LEAVE** the hazardous area immediately.

After reaching a hazard-free area, immediately remove the respirator.

DO NOT use a blower that fails the flow test.

Use **ONLY** Bullard cartridges which comply with and have the NIOSH approval label and which are appropriate for the contaminant.

Failure to observe these warnings could result in death or serious injury.



PA3ISBU Air-Purifying Elements

Principle of Operation

The following filter/cartridge protection classification applies when used with any of the hoods or loose fitting facepieces. In the following table "Quantity" refers to the number of filters/cartridges which must be attached to the blower unit to provide the required protection.

Protection	Filter/Cartridge Type	Quantity	NIOSH / ANSI Color Code for Cartridge Label
HE	PA3HE, PAPRFC1	2	Purple
OV/CL/HC/SD/CD/HF/HE	PA3OVAGHE, PAPRFC2	3	Yellow and Purple
CL/HC/SD/CD/HF/FM/AM/MA/HE	PA3NBC*	3	Olive Green and Purple

*The PA3NBC cartridge provides protection for acid gases, formaldehyde, and ammonia and therefore is effective against a wide range of Toxic Industrial Chemicals. The High Efficiency (HE) Particulate Filter provides protection against airborne bacteria, viruses, and other particulates. Although not NIOSH-approved for use against the following contaminants, independent laboratories have tested and verified that the PA3NBC cartridge is effective against many chemical warfare agents and/or their recognized surrogates. These agents/surrogates are listed below.

PA3NBC CARTRIDGE CHEMICAL WARFARE GAS PERFORMANCE TESTING				
Gas Challenge	Test Concentration	Flow Rate	Breakthrough Concentration	Time to Breakthrough
DMMP	3000 mg/m ³	50 lpm	.04 mg/m ³	>120 minutes*
Sarin (GB)	4000 mg/m ³	32 lpm	.04 mg/m ³	>120 minutes*
Cyanogen Chloride (CK)	4000 mg/m ³	32 lpm	8.0 mg/m ³	30 minutes*
Chloropicrin (PS)	15000 mg/m ³	30 lpm	0.7 mg/m ³	60 minutes
Hydrogen Cyanide (AC)	5500 mg/m ³	30 lpm	5.0 mg/m ³	>30 minutes
Tear Gas (CS)	23 mg/m ³	64 lpm	0.4 mg/m ³	>480 minutes
Tear Gas (CN)	101 mg/m ³	64 lpm	0.3 mg/m ³	>480 minutes

*These tests are part of the performance specifications for the C2A1 military canister. The PA3NBC Cartridge meets or exceeds the performance requirements of the C2A1 canister for these gases.

HE particulate filters are 99.97% effective against all particulate aerosols.

Filters and cartridges are supplied in quantities of six per box.

The following abbreviations are approved by NIOSH to indicate the particulates, gases or vapors which are removed by the gas/vapor cartridges:

CL	Chlorine
CD	Chlorine Dioxide
HC	Hydrogen Chloride
SD	Sulfur Dioxide
FM	Formaldehyde
AM	Ammonia
MA	Methylamine
OV	Organic Vapors
HF	Hydrogen Fluoride
HE	High Efficiency Particulate Air Filter for Powered Air-Purifying Respirators

⚠ WARNING

Use only the cartridge described in the above table. Used/particulate-laden cartridges must be changed as a set and not individually. All cartridges must be of the same type. Do not change cartridges while in a hazardous atmosphere. Incorrect cartridge selection will invalidate all performance statements and approvals for this equipment.

Three (3) of the same type of cartridge must be used on the PA3ISBU blower unit, with the exception of the PA3HE or PAPRFC1 filter which are used two (2) at a time, in conjunction with the PA3PG plug. DO NOT use the PA3PG plug to close off a port with any other cartridge type.

The PA3NBC cartridges and PA3BU blower should only be used with the 20SICVH and 20SICV hoods. These hoods are made of Tychem SL, which has been tested by DuPont and shown to be effective against chemical warfare agents. These hoods also feature a press polished vinyl lens adequate for hospital preparedness applications.

These respirators are not NIOSH-approved for use against chemical warfare agents.

The respirator and cartridges should not be used beyond eight (8) hours after initial exposure to chemical warfare agents to avoid possibility of agent permeation. If liquid exposure is encountered, the respirator should not be used for more than two (2) hours.

Follow established cartridge change schedules to ensure that cartridges are replaced before breakthrough occurs. Failure to follow these warnings could result in death or serious injury.

PA30IS Series Powered Air-Purifying Respirator PA3IS Blower Assembly User Manual

Mounting and Replacing Cartridges on the Blower Unit

The useful life of a chemical cartridge for vapors and gases will vary with the concentration and nature of the contaminant, the breathing rate of the respirator wearer, and ambient temperature and humidity.

The Occupational Safety and Health Administration (OSHA) regulations 29 CFR 1910.134 require that the employer must implement a change schedule when using Air-Purifying respirators for protection against gases and vapors, if there is no end-of-service-life indicator on the cartridges. The change schedule must be based on objective data that will ensure that the cartridges are replaced before the end of their service life. Factors to consider include workplace conditions such as contaminant concentration, relative humidity, temperature, work activities, respirator use pattern (e.g., continuous or intermittent use), presence of other contaminants, potential for contaminant migration/desorption, health effects of the gas or vapor, and the presence of any warning properties. Contact Bullard for further information on change-out schedules.

High efficiency particulate filters must be replaced when retained particles clog the filters and reduce air flow below acceptable levels, as indicated by testing with the Air Flow Indicator.

To Replace Cartridges

Remove the air-purifying element from its packaging, and inspect for damage. If in doubt do not use.

Check that the air-purifying element has not exceeded its "use-by" date and that the connecting thread is in good condition.

Check that the air-purifying element is appropriate to the hazard. If in doubt consult your respirator program administrator or supervisor.

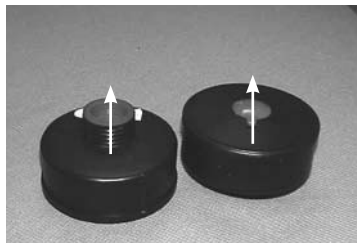


Figure 4

Check that the threads in the blower unit port are in good condition and clear of contaminant.

Check that the PA3ISBU blower ports have the rubber gasket seals present.

Remove the air-purifying element seals (see Figure 4).

Screw the air-purifying elements into the receptacles (see Figure 5) until the cartridge is hand tight. **DO NOT OVER-TIGHTEN.**

When using the two PA3HE filter cartridges, install the filter plug into one of the ports. **DO NOT OVER-TIGHTEN** (Figure 6).



Figure 5



Figure 6

Donning the Blower and Respirator

Prepare to don the blower, battery and hood in a safe, hazard-free area and do the following:

Check that the cartridges are properly mounted on the blower unit.

Prior to assembling the system, place the battery in the battery compartment on the back of the blower. Make sure that the correct battery is used in the appropriate blower unit. (See instructions and warning on page 2). Fit the blower and belt around the user's waist. With the blower at the rear of the user, adjust the belt for a comfortable fit.

Remove the belt and blower.

Ensure that the cartridges used are suitable for the contaminant in question and are compatible with the PA3ISBU Blower Unit.

⚠ WARNING

The use of any cartridge not approved with the PA3ISBU blower units may put the user at risk and could result in death or serious injury.

For Hoods:

Insert the PA1BT Breathing Tube approximately 5 inches into the air entry sleeve at the rear of the hood being used (see Figure 7).

Install nylon clamp S18051 over air entry sleeve and breathing tube, inserting clamp locks through two holes in plastic anchor plate that is sewn into hood (RT Hoods DO NOT have a plastic anchor plate.).

Engage clamp locks and squeeze together until tight.

For Loose Fitting Facepieces:

If the loose fitting facepiece hood is being used, insert the bayonet connector of the PA20LFBT Breathing Tube into the hood connector and turn clockwise until it locks in place (see Figure 8).

For All Headpieces:

Attach the other end of breathing tube to blower unit by screwing adapters together.

Remove any protective film covering the visor of the hood.

Put on the belt and blower assembly and make any final adjustments to the belt as necessary, keeping the breathing tube and hood behind the head.

Switch ON the blower.

Place the hood on the head making any final adjustments to the fit as required at this time to ensure a comfortable and stable fit.




Figure 7



Figure 8

⚠ WARNING

Do not enter a hazardous area until you are sure that the blower and hood are fully operational and the blower is running. The user should periodically leave the hazardous area to check the airflow through the system. If the PA3ISBU voltage Alarm should sound, or if the user experiences any difficulty in breathing, or senses any taste or any odors from the hazard, the user should leave the hazardous area immediately. Failure to observe these warnings could result in death or serious injury.

PA3ISBU Low Voltage Alarm

The PA3ISBU Blower units are equipped with a Low Voltage Alarm. This device will activate if the battery voltage is below acceptable levels. The PA3ISBU Low Voltage Alarm is a mechanical pulsing of the blower. The alarm is internal to the blower and the sound will be carried up the breathing tube into the hood. Sounding of the alarm indicates that insufficient airflow may be imminent. The user should immediately do the following:

Leave the hazard area, remove the headpiece, disconnect the breathing tube from the hood and check the airflow with the airflow indicator (see page 5).

If the airflow indicator indicates insufficient airflow, the battery should be fully charged (see "Battery Pack" on page 4), and/or the filter/cartridge should be replaced.

The PA3ISBU Low Voltage Alarm must not be solely relied upon as an indication of a low air flow condition. Only the Air Flow Indicator should be utilized for checking for adequate air flow, as required by NIOSH.

NOTE

When the Low Voltage Alarm sounds and the filter cartridges are not clogged, the battery should be recharged to protect the battery and thereby prolong the working life of the unit. If the ball in the Airflow Indicator is **BELOW** or **PARTLY BELOW** the **PASS LINE** with a fully charged battery, the filter cartridges may need to be changed.

Troubleshooting

The following guide will enable you to locate and correct malfunctions:

Malfunction	Possible Cause	Solution
Low Voltage Alarm is sounding, but Airflow Indicator shows adequate air flow or breathing tube inserted incorrectly	Low Voltage Air inlet to hood is twisted or constricted,	Re-charge battery Remove, inspect, and reinsert PA1BT Breathing Tube approximately 5" into hood inlet.
No/low airflow into covering (Alarm sounding for low voltage)	Clogged/damaged air-purifying filter element Battery low Blower malfunction Breathing tube or hood damaged	Replace the filter cartridge. Re-charge battery. Replace blower. Replace breathing tube and/or hood.
Smell or taste contaminant	Equipment damaged or filter needs to be replaced Low airflow	Leave hazardous area immediately and check equipment. Replace filter. If the problem persists and no damage is found, return equipment for repair. See above.
Blower unit does not run for full service life PA3IS (Approximately 7 hours with 1 battery pack)	Improper initial charge Prolonged storage of unit not on charger Deeply discharged battery	Review "Initial Charging Procedure" on page 3. Review guidelines for maximizing battery life, page 2 (under Battery Pack)

WARNING

Avoid contaminant entry into the breathing tube, as this will compromise respiratory protection and could result in death or serious injury. Consult your local safety professional if you suspect that contaminant has entered the breathing tube. When cleaning the equipment, do the following:
Ensure water does not enter cartridges. Replace wet cartridges.
DO NOT use gasoline, organic-based solvents, or chlorinated degreasing fluids (such as trichloroethylene) as they will cause damage.
DO NOT immerse the equipment in water or other cleaning fluid as this may cause contamination in the breathing tube and blower interior that will be difficult to remove.
Failure to observe the instructions and warnings in this manual invalidates all performance statements and approvals for this equipment and could result in death or serious injury.

Cleaning

Once cartridges have reached the end of their useful life, discard in accordance with federal, state, and local guidelines, and in conformance with plant safety regulations.

Use a lint-free cloth moistened in a mild solution of soap and warm water to clean the outer surface of the equipment.

Consult the CC20/RT Series Tychem Hood User Manual for cleaning instructions for the hood components.

Storage

When the apparatus is completely dry, store in a clean, dry area, away from direct sunlight and sources of direct heat.

The storage temperature should be between 32° F to 90° F (0° C to 32° C) with humidity less than 90% RH.

Consult the CC20 Series Hood User Manual or RT Series Hood User Manual for storage instructions on hood components.

Ordering Information

CATALOG NUMBER	DESCRIPTION
Respirator Assemblies	
PA30ISLFLSB	20LFL Loose-Fitting Facepiece System with Standard Comfort Belt
PA30ISTJJB	20TJ Single Bib Hood System with Standard Comfort Belt
PA30ISTICSB	20TIC Double Bib Hood System with Standard Comfort Belt
PA30ISTICHSB	20TICH Double Bib Hood for Hard Hat System with Standard Comfort Belt
PA30ISSICSB	20SIC Double Bib Saranex Coated Hood System with Standard Comfort Belt
PA30ISSICHSB	20SICH Double Bib Saranex Coated Hood For Hard Hat System with Standard Comfort Belt
PA30ISTPSB	20TP Single Bib Hood for Painting System with Standard Comfort Belt
PA30ISTPCSB	20TPC Double Bib Hood for Painting System with Standard Comfort Belt
PA30ISTICSSB	20TICS Extra Long Double Bib Hood System with Standard Comfort Belt
PA30ISRTISB	RT1 Headband Free Extra Large Lens Double Bib Hood System with Standard Comfort Belt
PA30ISRT2SB	RT2 Headband Free Extra Large Lens Double Bib Saranex Coated Hood System with Standard Comfort Belt
PA30ISRT3SB	RT3 Headband Free Extra Large Lens Double Bib Hood System with Standard Comfort Belt
PA30ISRT4SB	RT4 Headband Free Extra Large Lens Double Bib Hood System with Standard Comfort Belt



NOTE

For Decon Belt change SB suffix to DB

Blower Assemblies

PA3IS	Tri-filter blower unit (blue color), intrinsically safe with low voltage alarm, battery, and belt. Breathing tube, replacement battery and charger sold separately.
-------	---

Battery Chargers

PA3ISC	Quick charger for PA3ISBP (1 port)
PA3ISGC	Table top gang charger (6 ports)

Replacement Cartridges

PAPRFC2	OV/CL/HC/SD/CD/HF/HE (6 per box)
PAPRFCL	HE (6 per box)
PA3HE	HE (6 per box)
PA3OVAGHE	OV/CL/HC/SD/CD/HF/HE (6 per box)
PA3NBC	CL/HC/SD/CD/HF/FM/AM/MA/HE (6 per box)

Respirator Hoods

Basic style hood, for use with headband suspension

20TJ	Tychem QC with 20TG headband suspension
20TJN	Tychem QC, no headband suspension
20TP	Tychem QC, with solvent-resistant polyester lens, 20TG headband suspension (CC20 only)
20TPN	Tychem QC with solvent-resistant polyester lens, no suspension (CC20 only)

Hood with inner bib, for use with headband suspension

20TIC	Tychem QC, with 20TG headband suspension
20TICN	Tychem QC, no headband suspension
20TPC	Tychem QC, with solvent-resistant polyester lens, 20TG headband suspension (CC20 only)
20TPCN	Tychem QC with solvent-resistant polyester lens, no suspension (CC20 only)

Hood with inner bib, for use with Bullard hard hat

20TICH	Tychem QC, hard hat not included
20SICH	Tychem SL, with taped and sealed seams, hard hat not included
20SICVH	Tychem SL, with taped and sealed seams and CBRN-resistant PVC lens, hard hat not included

CATALOG NUMBER	DESCRIPTION
Hood with inner bib and long outer bib, for use with headband suspension	
20TICS	Tychem QC with taped and sealed seams, and 20TG headband suspension
20TICSN	Tychem QC with taped and sealed seams, no headband suspension
20SIC	Tychem SL, with taped and sealed seams, and 20TG headband suspension
20SICN	Tychem SL, with taped and sealed seams, no headband suspension
20SICVN	Tychem SL, with taped and sealed seams and CBRN-resistant PVC lens, no headband suspension

Hoods with Inner Bib and Long Outer Bib, for use without a Suspension

RT1	Tychem QC Hood with long inner and outer bib (inflatable neck cuff)
RT2	TychemSL Hood with long inner and outer bib (inflatable neck cuff)
RT3	Tychem QC Hood with long inner and outer bib (sport neck cuff)
RT4	Tychem SL Hood with long inner and outer bib (sport neck cuff)

Loose Fitting Facepieces with Sewn-In Suspension

20LFM	Tychem QC, facial seal, medium
20LFL	Tychem QC, facial seal, large
20LF2S	Tychem QC, facial seal, narrow profile, small
20LF2M	Tychem QC, facial seal, narrow profile, medium
20LF2L	Tychem QC, facial seal, narrow profile, large

Accessory Items for All Hoods

20LCL	Mylar lens covers (25/pkg)
-------	----------------------------

Headband Suspensions and Hard Hats

20TG	Standard headband suspension
20RT	Sure-Lock® ratchet headband suspension
30XXP	Hard hat with standard suspension
30XXR	Hard hat with ratchet suspension
51XXP	Hard hat with standard suspension
51XXR	Hard hat with ratchet suspension

Accessories for Headbands Suspension and Hard Hats

ESULTRA	Standard replacement suspension for C30 hard hat
ESRTSL	Replacement ratchet suspension for C30R hard hat
RS4PC	Standard replacement suspension for S51R hard hat
RS4RC	Replacement ratchet suspension for S51R hard hat
20NC	Chin strap for 20TG and 20RT headband suspension
ES42	Chin strap for 3000 and 5100 hard hats

Replacement Parts and Accessories

PAISB	Standard belt
PAIDB	Decon belt
PAIEB	Extension standard belt kit
PAIDEB	Extension decon belt kit
PAIAFI	Air flow indicator
PA3ISBU	Blower housing unit (I.S. version), motor and impeller
PAIBT	Hood breathing tube assembly; includes tube and clamp; standard length
PAIBTXS	Hood breathing tube assembly; includes tube and clamp; short length
PA20LFBTXL	Loose fitting facepiece breathing tube assembly; extra long length
PA20LFBT	Loose fitting facepiece breathing tube assembly; standard length
PA20LFBTXS	Loose fitting facepiece breathing tube assembly; short length
PAIBTS	Breathing tube/cartridge seal
PA3ISBP	7 hour battery pack (Intrinsically Safe)
S18051	Breathing tube clamp
PA3PG	Plug for blower port

Americas:

E.D. Bullard Company
 1898 Safety Way
 Cynthiana, KY 41031-9303
 Toll free: 877-BULLARD (285-5273)
 Tel: 859-234-6616
 Fax: 859-234-8987
www.bullard.com

Europe:

Bullard GmbH
 Lilienthalstrasse 12
 53424 Remagen • Germany
 Tel: +49-2642 999980
 Fax: +49-2642 9999829
www.bullardextrem.com

Asia-Pacific:

Bullard Asia Pacific Pte. Ltd.
 LHK Building
 701, Sims Drive, #04-03
 Singapore 387383
 Tel: +65-6745-0556
 Fax: +65-6745-5176
www.bullard.com

©2009 Bullard. All rights reserved.
 Tychem is a registered trademark of E.I. DuPont de Nemours & Company.



ISO 9001
 certified